

## ChromIQ Analytical Laboratory


HPLC-MS Quality Control &amp; Peptide Purity Analysis

Website: chromiq.com | Email: qc@chromiq.com

## PRODUCT DATA

Product	<b>Bacteriostatic Water (10 mL)</b>	Batch	<b>BAC10-B0262</b>
CAS	7732-18-5	Formula	H2O
Appearance	Clear, colorless sterile solution	Mol. Wt.	—
Quantity	10 mL / vial	Purity	<b>99.65%</b>
Content	Benzyl alcohol 0.89% w/v	Analysis Method	GC-FID, benzyl alcohol assay (per spec)   Column: DB-WAX, 30 m x 0.32 mm   Carrier: H2   Inj.: 1.0 µL split 50:1
Analysis Conducted	2026-05-22	Principal Chemist	Dr. Marek Janowski, Ph.D.
Produced	2026-05-20	Storage	Store at 15-30 °C, do not freeze
QC Status	PASS — conforms to specification	Report No.	CIQ-RPT-B0262

## GC-FID CHROMATOGRAM

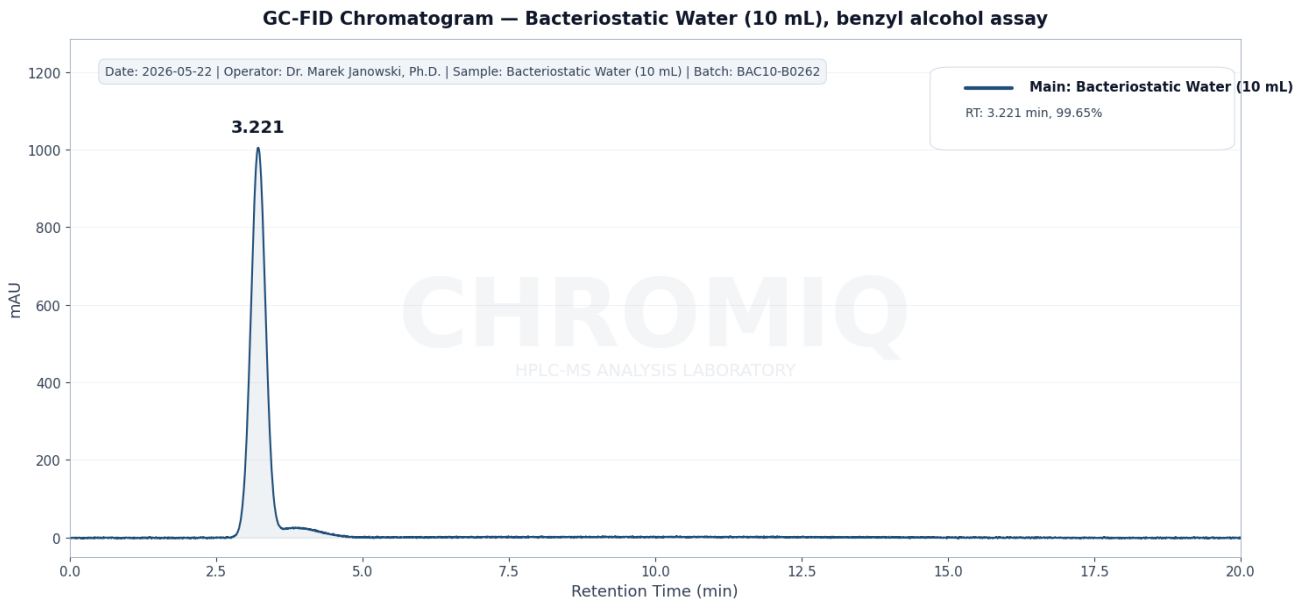

Method: GC-FID, benzyl alcohol assay (per spec) | Column: DB-WAX, 30 m x 0.32 mm | Carrier: H2 | Inj.: 1.0 µL split 50:1

Signal: FID Detector: GC-FID

Carrier Gas: H2 | Injector: 250 °C | Detector: 280 °C

Dr. Marek Janowski, Ph.D.

Principal Chemist · 2026-05-22

A. Reynolds, QA Manager

Quality Assurance · 2026-05-23

This certificate applies only to the batch identified above. For laboratory and research use only — not for human or veterinary use, diagnosis, or therapeutic application. © ChromIQ Analytical Laboratory · chromiq.com